Gold Standard Analytics

Gold Standard Analytics LLC, Houston, TX

CERTIFICATE OF ANALYSIS

Report GSA-COA-000141-14104-20261126 · issued Nov 26, 2026

Mark Miscione

PRODUCT	ORDER	SAMPLE
Retatrutide	GSA-2026-000141	141-04
LABEL	**LOT**	**ISSUED**
Skynet Peptides, Retatrutide 50 mg	04SP42001	Nov 26, 2026

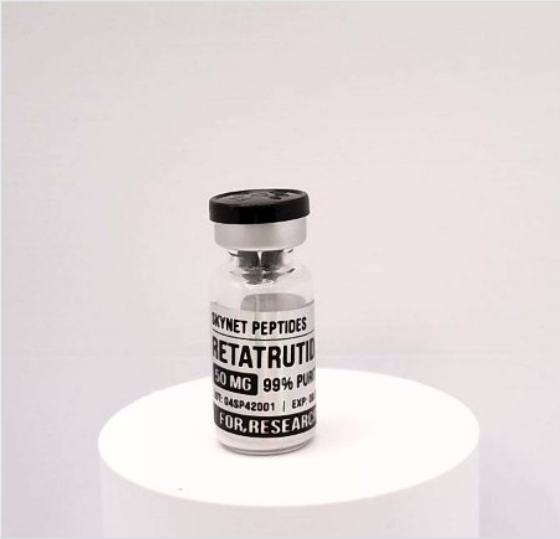

THE SAMPLE AS RECEIVED

IDENTITY ✓

Retatrutide

confirmed by mass

PURITY ✓

99.51 %

HPLC-UV, 214 nm

HPLC CHROMATOGRAM — UV, 214 nm

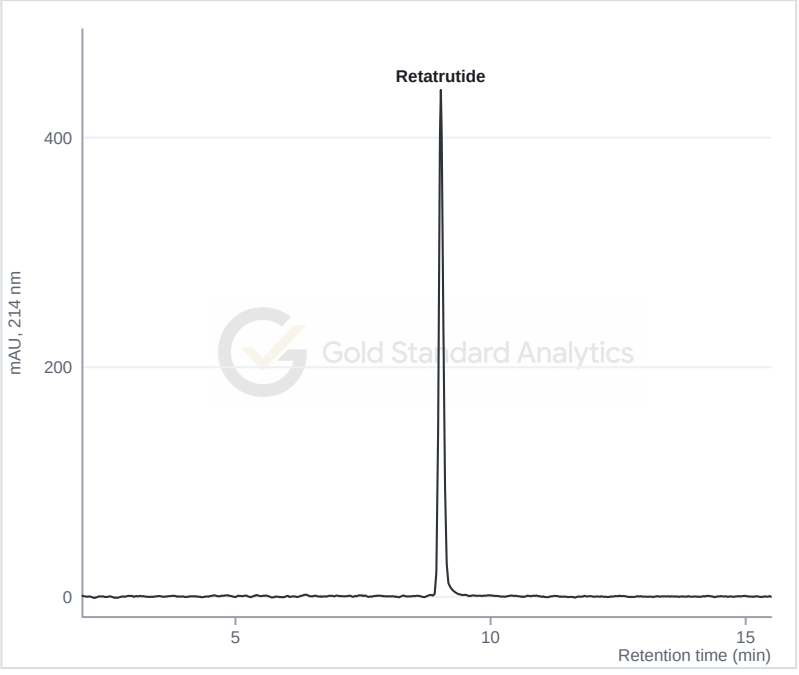

MASS SPECTRUM — at the retatrutide peak (9.03 min)

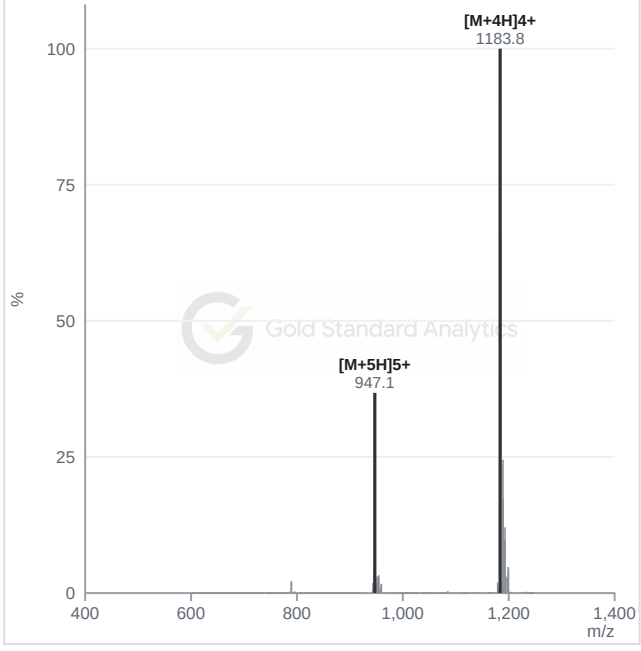

RELEASED BY

Ian Ebert

Chemist & Lab Lead · Nov 27, 2026

Scan to verify

goldstandardanalytics.com/coa/

Results are not covered by ISO/IEC 17025 accreditation. Results relate only to the sample as received and tested.

The sample

Order GSA-2026-000141 · Sample 141-04 · Mark Miscione

Customer	**Mark Miscione**	Lot	**04SP42001**
Order	**GSA-2026-000141**	Prepared	**25 Nov 2026**
Sample	**141-04**	Tested	**26 Nov 2026**
Label	**Skynet Peptides, Retatrutide 50 mg**	Tests	**Identity, Purity**

Graphs

HPLC CHROMATOGRAM

HPLC chromatogram (UV, 214 nm) · mAU, 214 nm against Retention time (min)

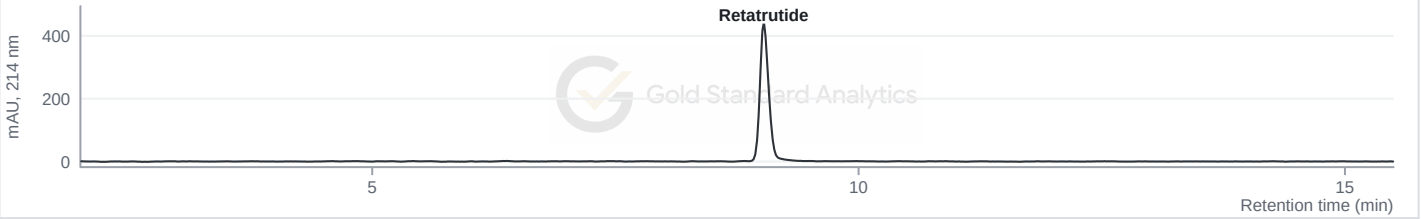

MASS SPECTRUM

Mass spectrum at the retatrutide peak (9.03 min) · Counts against m/z

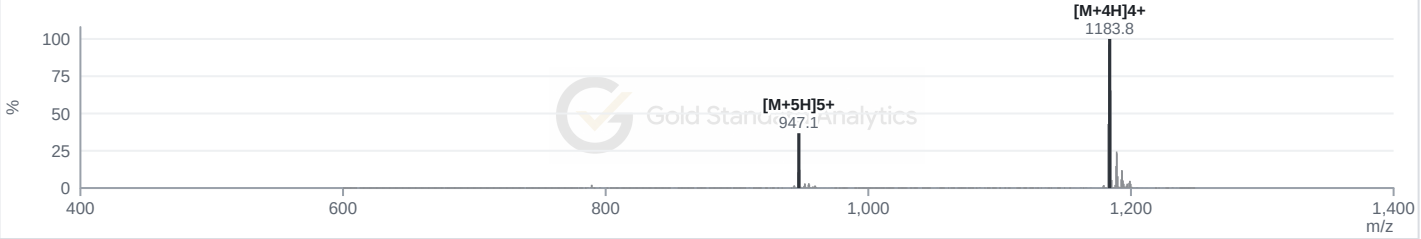

Results

Identity	**Consistent with retatrutide.** The main peak at 9.03 min carries retatrutide's 4+ and 5+ ions (m/z 1183.8 and 947.1; molecular mass 4,730.6, expected 4,731.3).
Purity	**99.51 %** by HPLC with UV detection at 214 nm. No peak other than retatrutide was found, down to about 0.49 % of the retatrutide peak height, so purity is reported as 99.51 % rather than as 100 %.

Zoomed views

HPLC, SMALL PEAKS

Zoomed in on the small peaks (5 % of the main peak) · mAU, 214 nm against Retention time (min)

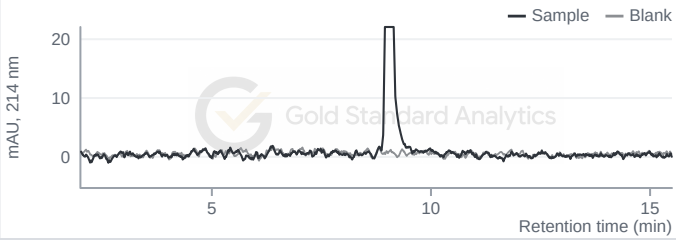

ION TRACE

Ion trace, m/z 1183.8 (retatrutide 4+): sample vs blank · Counts against Retention time (min)

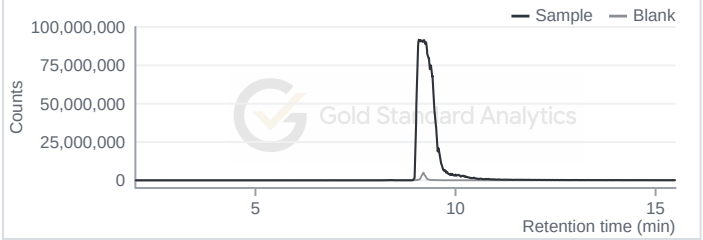

How it was tested

Liquid chromatography with UV and mass-spectrometry detection: Agilent 1290 Infinity II LC with a 6490 triple-quadrupole mass spectrometer. Column Polaris C18-A, 2.0 x 150 mm, 55 °C; water and acetonitrile, each with 0.1 % formic acid. Identity: molecular mass from the multiply charged ions in the mass spectrum. Purity: UV peak area at 214 nm, after subtracting a blank run in the same sequence. 0.7 µL injected; autosampler at 12 °C.

Notes

Results apply only to the sample as received and tested.

Release

This report is signed electronically at release. The signature is printed on page 1, and the release record, added as the last page, gives the date and the verification code.

Gold Standard Analytics

goldstandardanalytics.com

Release record

Report GSA-COA-000141-14104-20261126 · Certificate GSA-2026-474152

Customer and order	Mark Miscione · GSA-2026-000141
Sample and report	141-04 · Retatrutide Certificate of Analysis
Report reference	GSA-COA-000141-14104-20261126
Certificate accession	GSA-2026-474152
Released and signed by	Ian Ebert, Chemist & Lab Lead
Date and time (UTC)	2026-11-27 06:59:13Z
Signature meaning	Approved for release. The signer reviewed this report and approved its release to its customer.
Approval reference	374a9061-5d25-4cb1-b0fd-320f1e4907b7
Electronic signature	Signed electronically in a signed-in GSA staff account.
Original report SHA-256	591e6f8c4e84a8e7cec0e84bbb845589505453231fb65e9bdb1d6b9dd046de82
Verify this certificate	https://goldstandardanalytics.com/coa/GSA-2026-474152

Scan to view this certificate online

Signature

Ian Ebert, Chemist & Lab Lead

Results are not covered by ISO/IEC 17025 accreditation.
Results relate only to the sample as received and tested.