Gold Standard Analytics

Gold Standard Analytics LLC, Houston, TX

CERTIFICATE OF ANALYSIS

Report GSA-COA-CUST-LA-BPCCAPS-20261112-5 · issued Nov 18, 2026

LA Peptides

PRODUCT
BPC-157 capsules

ORDER
Custom sample

SAMPLE
LA-BPCCAPS-20261112

LABEL
BPC 157 capsule

ISSUED
Nov 18, 2026



THE SAMPLE AS RECEIVED

IDENTITY ✓
BPC-157
confirmed by mass

PURITY ✓
100 %
HPLC-UV, 214 nm


FENTANYL SCREEN ✓
Not detected
fentanyl and 15 related compounds

ENDOTOXINS ✓
< 0.050 EU/mL
Pass; spike recovery 94 %

✓ **Sterility**	Pass; both canisters, 14 days	**No growth**	
✓ **Heavy metals**	USP <232>, ICP-MS: Pb, Cd, Hg, As, Co, V, Ni	**Pass**	


HPLC CHROMATOGRAM

UV, 214 nm

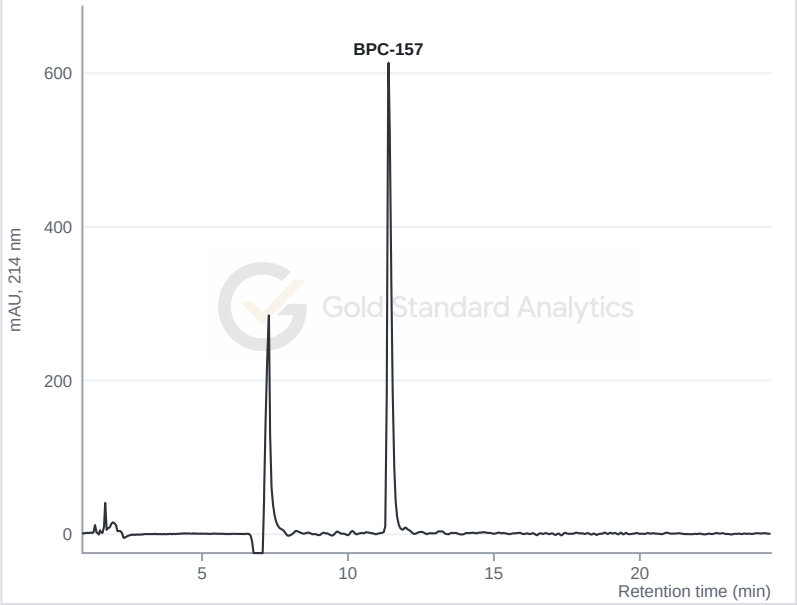

MASS SPECTRUM

main peak (11.39 min)

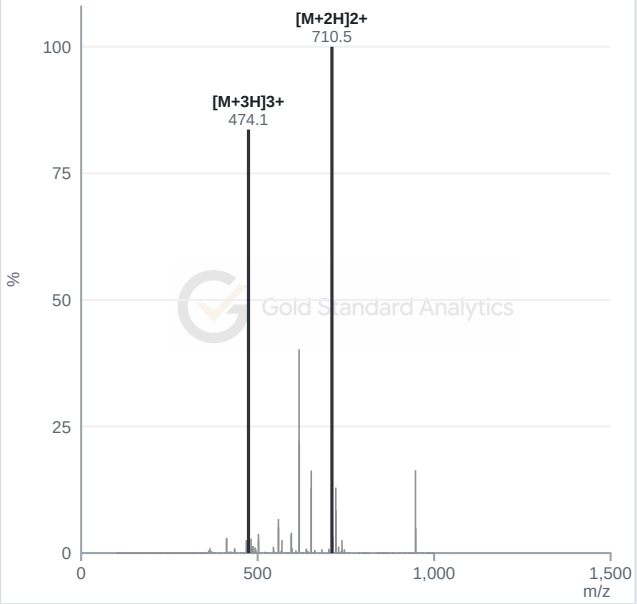

RELEASED BY

Ian Ebert
Laboratory Director · Nov 19, 2026

Scan to verify
goldstandardanalytics.com/coa/

Results are not covered by ISO/IEC 17025 accreditation. Results relate only to the sample as received and tested.

The sample


Custom sample · LA Peptides

Customer	**LA Peptides**	Prepared	**Capsule contents dissolved and filtered to remove the filler, 11 Nov 2026**
Order	**Custom sample**	Tested	**12 Nov 2026**
Sample	**LA-BPCCAPS-20261112**	Tests	**Identity, Purity, Impurity breakdown, Fentanyl screen, Bacterial endotoxins, Sterility, Elemental impurities**
Label	**BPC 157 capsule**		

Graphs


HPLC CHROMATOGRAM

HPLC chromatogram (UV, 214 nm) · mAU, 214 nm against Retention time (min)

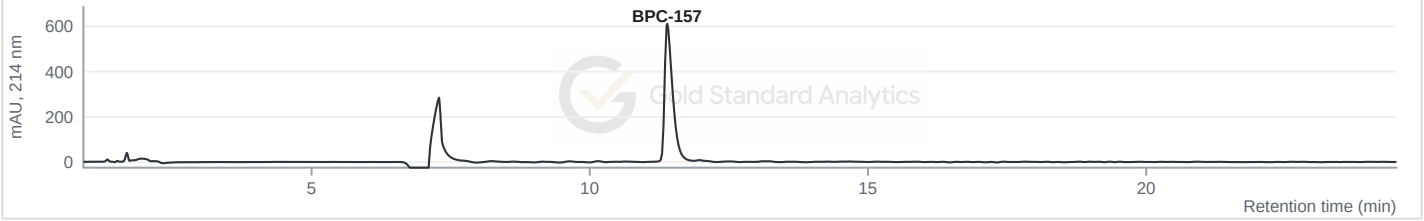

MASS SPECTRUM

Mass spectrum of the main peak (11.39 min) · Counts against m/z

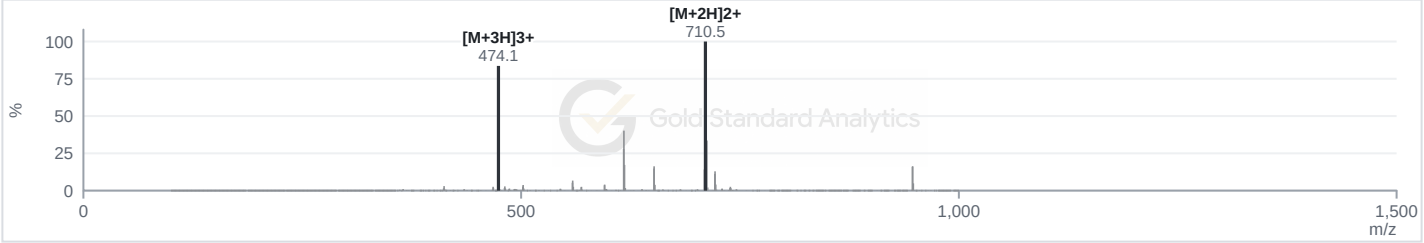


Results

Identity	**Consistent with BPC-157.** The main peak at 11.39 min carries BPC-157's 2+ and 3+ ions (m/z 710.5 and 474.1); measured mass 1,419.1 (expected 1,419.5).
Purity	**100 %** by HPLC with UV detection at 214 nm: no other peak was found above the reporting limit (about 1.3 % of the BPC-157 peak height). The capsule also contains arginine and a sugar alcohol such as mannitol (common capsule ingredients), seen by mass at the start of the run; neither is a peptide and neither is counted in purity. The large peak at about 7.3 min in the chromatogram comes from the instrument, not the sample: the same peak appears when only blank solvent is injected.
Fentanyl screen	**Not detected.** The capsule solution was screened by LC-MS/MS (multiple-reaction monitoring, two ion transitions each) for fentanyl and 15 related compounds: norfentanyl, 4-ANPP, acetylfentanyl, acrylfentanyl, butyrylfentanyl, cyclopropylfentanyl, furanylfentanyl, methoxyacetylfentanyl, para-fluorofentanyl, ocfentanil, carfentanil, sufentanil, alfentanil, remifentanil and valerylfentanyl. This is a screen: no detection limit is stated.
Bacterial endotoxins	**< 0.050 EU/mL; spike recovery 94%** . Pass.
Sterility	**No growth in either canister after 14 days** . Pass.
Elemental impurities (USP <232>)	**Pb < 0.5 µg/g; Cd < 0.2 µg/g; Hg < 0.3 µg/g; As < 1.5 µg/g; Co < 5 µg/g; V < 10 µg/g; Ni < 20 µg/g (Agilent ICP-MS)** . Pass.

Zoomed views


HPLC, SMALL PEAKS

Zoomed in on the small peaks · mAU, 214 nm against Retention time (min)

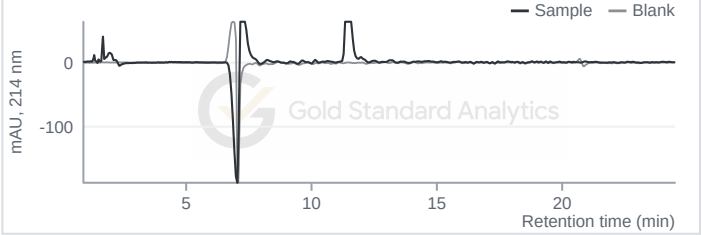

ION TRACE

Ion trace, m/z 710.4 (BPC-157 2+): sample vs blank · Counts against Retention time (min)

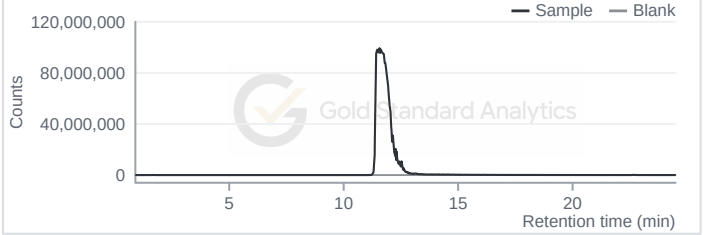

Impurities

Every UV peak above the reporting limit was BPC-157.

Amounts are each peak's share of the total UV peak area at 214 nm.

How it was tested

Liquid chromatography with UV and mass-spectrometry detection: Agilent 1290 Infinity II LC with a 6490 triple-quadrupole mass spectrometer. Column Polaris C18-A, 2.0 x 150 mm, 45 °C; water and acetonitrile, each with 0.1 % formic acid. Purity: UV peak area at 214 nm, after subtracting a blank run in the same sequence. Identity: molecular mass from the mass spectrum. Fentanyl screen: a separate injection with LC-MS/MS in multiple-reaction-monitoring mode. Bacterial endotoxins: endotoxin reader, 0.050 EU/mL limit; result reported as printed by the reader, with spike recovery. Sterility: membrane filtration (canisters), 14-day incubation. Elemental impurities (USP <232>): Agilent ICP-MS; Pb, Cd, Hg, As, Co, V, Ni.

Notes

Results apply only to the sample as received and tested.

Release

This report is signed electronically at release. The signature is printed on page 1, and the release record, added as the last page, gives the date and the verification code.

Gold Standard Analytics

goldstandardanalytics.com

Release record

Report GSA-COA-CUST-LA-BPCCAPS-20261112-5 · Certificate GSA-2026-578889

Customer and order	LA Peptides · Custom sample (no order)
Sample and report	LA-BPCCAPS-20261112 · BPC-157 capsules Certificate of Analysis
Report reference	GSA-COA-CUST-LA-BPCCAPS-20261112-5
Certificate accession	GSA-2026-578889
Released and signed by	Ian Ebert, Laboratory Director
Date and time (UTC)	2026-11-19 20:37:21Z
Signature meaning	Approved for release. The signer reviewed this report and approved its release to its customer.
Approval reference	bef71049-8c58-4edc-a751-35ac41d2d9c1
Electronic signature	Signed electronically in a signed-in GSA staff account.
Original report SHA-256	2d5a3103b7ecbd4e8f0437d7429ff597cccf5e44a115e18b888282af1a83357f
Verify this certificate	https://goldstandardanalytics.com/coa/GSA-2026-578889

Scan to view this certificate online

Signature

Ian Ebert, Laboratory Director

Results are not covered by ISO/IEC 17025 accreditation.
Results relate only to the sample as received and tested.