Gold Standard Analytics

Gold Standard Analytics LLC, Houston, TX

CERTIFICATE OF ANALYSIS

Report GSA-COA-000097-09701-20261116 · issued Nov 17, 2026

Vertinox Labs

PRODUCT	ORDER	SAMPLE
Retatrutide	GSA-2026-000097	097-01
LABEL	**LOT**	**ISSUED**
RETRATUTIDE, PB-2026-RET-8102	PB-2026-RET-8102	Nov 17, 2026

THE SAMPLE AS RECEIVED

IDENTITY

Retatrutide

confirmed by mass and retention time


PURITY

100 %

HPLC-UV, 214 nm


HPLC CHROMATOGRAM

UV, 214 nm

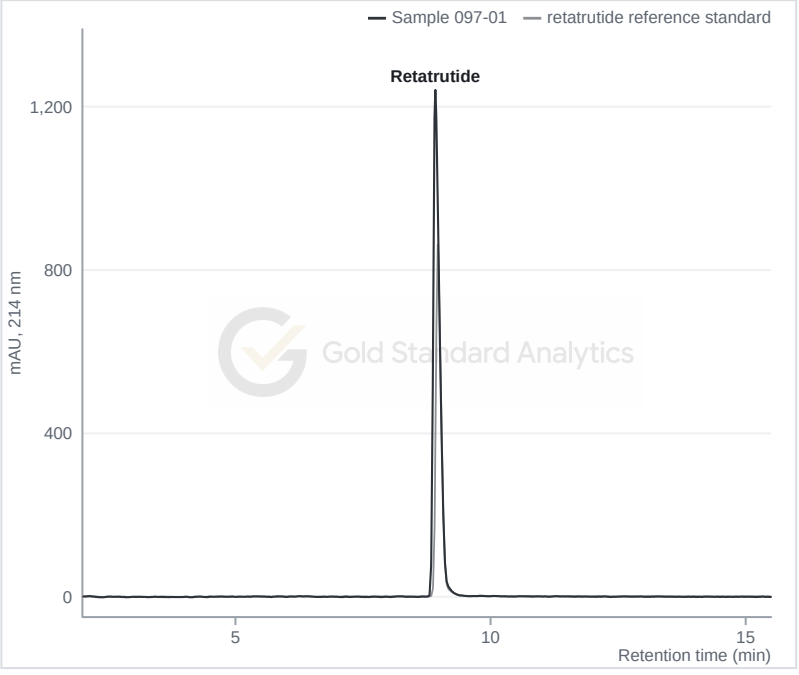

MASS SPECTRUM

at the retatrutide peak (8.92 min)

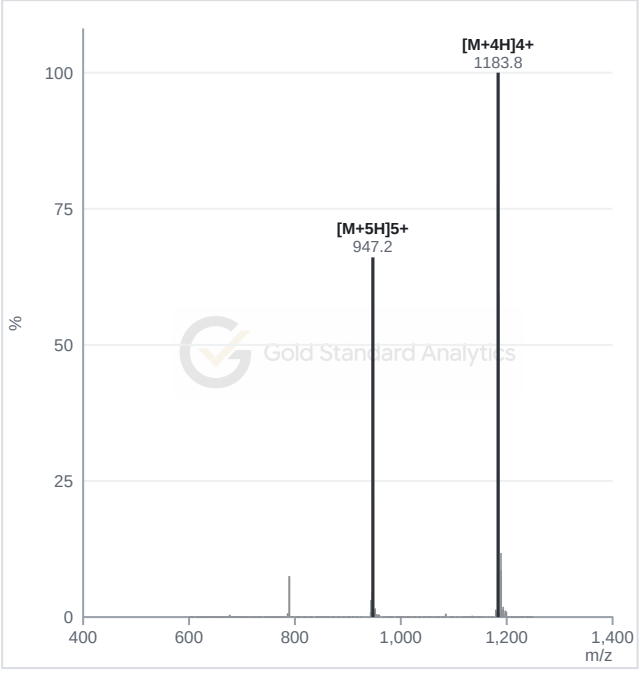

RELEASED BY

Ian Ebert

Laboratory Director · Nov 17, 2026

Scan to verify

goldstandardanalytics.com/coa/

Results are not covered by ISO/IEC 17025 accreditation. Results relate only to the sample as received and tested.

The sample


Order GSA-2026-000097 · Sample 097-01 · Vertinox Labs

Customer	**Vertinox Labs**	Lot	**PB-2026-RET-8102**
Order	**GSA-2026-000097**	Prepared	**16 Nov 2026**
Sample	**097-01**	Tested	**16 Nov 2026**
Label	**RETRATUTIDE, PB-2026-RET-8102**	Tests	**Identity, Purity**

Graphs


HPLC CHROMATOGRAM

HPLC chromatogram (UV, 214 nm) · mAU, 214 nm against Retention time (min)

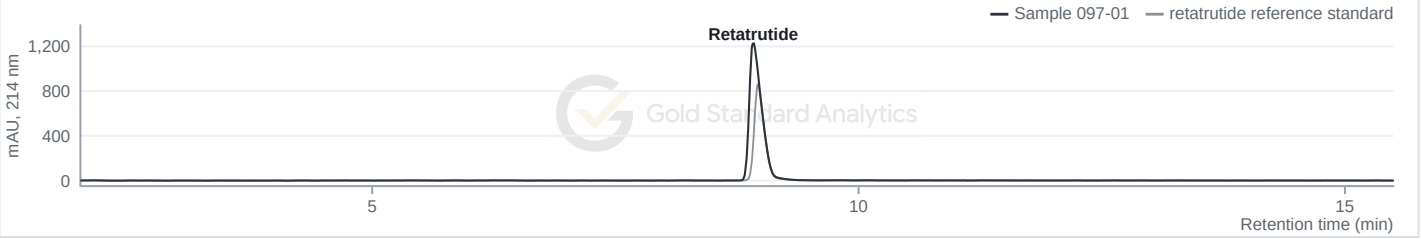

MASS SPECTRUM

Mass spectrum at the retatrutide peak (8.92 min) · Counts against m/z

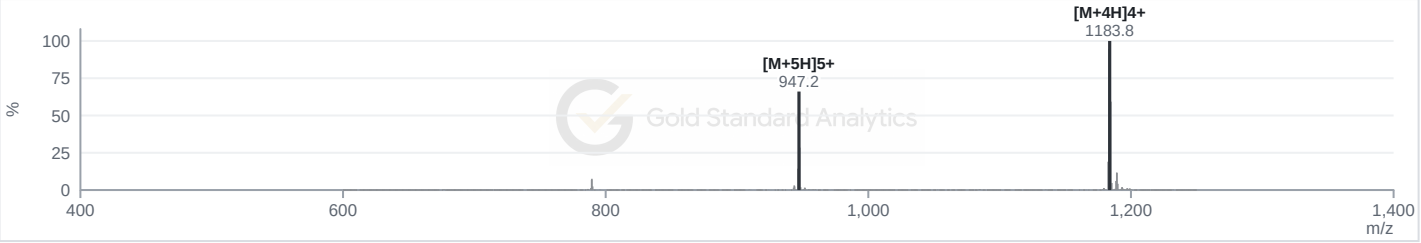


Results

Identity	**Consistent with retatrutide.** The main peak at 8.92 min carries retatrutide's 4+ and 5+ ions (m/z 1183.8 and 947.2; molecular mass 4,731.1, expected 4,731.3) and elutes within 0.5 % of a retatrutide reference standard run in the same sequence (8.97 min).
Purity	**100 %** by HPLC with UV detection at 214 nm: no other peak was found above the reporting limit (about 0.2 % of the retatrutide peak height).

Zoomed views


HPLC, SMALL PEAKS

Zoomed in on the small peaks (5 % of the main peak) · mAU, 214 nm against Retention time (min)

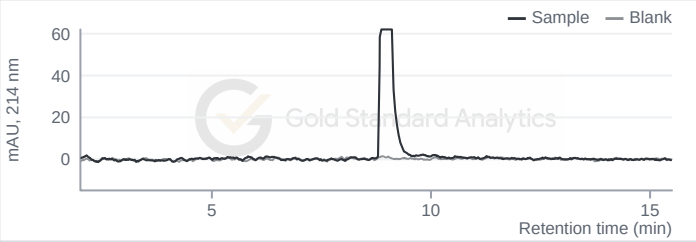

ION TRACE

Ion trace, m/z 1183.8 (retatrutide 4+): sample vs blank · Counts against Retention time (min)

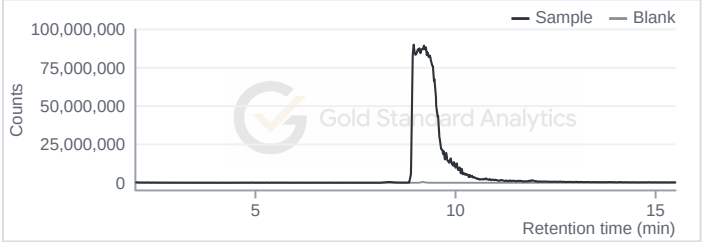

How it was tested

Liquid chromatography with UV and mass-spectrometry detection: Agilent 1290 Infinity II LC with a 6490 triple-quadrupole mass spectrometer. Column Polaris C18-A, 2.0 x 150 mm, 55 °C; water and acetonitrile, each with 0.1 % formic acid. Identity: molecular mass from the multiply charged ions in the mass spectrum, and retention time against a retatrutide reference standard run in the same sequence. Purity: UV peak area at 214 nm, after subtracting a blank run in the same sequence. 2 µL injected; autosampler at 12 °C.

Notes

Results apply only to the sample as received and tested.

Release

This report is signed electronically at release. The signature is printed on page 1, and the release record, added as the last page, gives the date and the verification code.

Gold Standard Analytics

goldstandardanalytics.com

Release record

Report GSA-COA-000097-09701-20261116 · Certificate GSA-2026-988675

Customer and order	Vertinox Labs · GSA-2026-000097
Sample and report	097-01 · Retatrutide Certificate of Analysis
Report reference	GSA-COA-000097-09701-20261116
Certificate accession	GSA-2026-988675
Released and signed by	Ian Ebert, Laboratory Director
Date and time (UTC)	2026-11-17 19:36:09Z
Signature meaning	Approved for release. The signer reviewed this report and approved its release to its customer.
Approval reference	645b8ef4-9777-47a3-adb9-123f2ca06ae5
Electronic signature	Signed electronically in a signed-in GSA staff account.
Original report SHA-256	6af0a86cff40cace66a19036fbb09cc11cbc8b28fcdd8391a4812ac1d6927cfe
Verify this certificate	https://goldstandardanalytics.com/coa/GSA-2026-988675

Scan to view this certificate online

Signature

Ian Ebert, Laboratory Director

Results are not covered by ISO/IEC 17025 accreditation.
Results relate only to the sample as received and tested.